

Pasteurisers for Donor Human Milk & Special Diets



PASTEURISATION OF DONOR HUMAN MILK for premature and other infants provides the best protection for the prevention of infections. Donor Human Milk is the preferred feed when mother's own milk is not available. Pasteurisation of human milk facilitates the retention of immunological factors and eliminates HIV (Aids) virus.

STERIFEED Pasteurisers comply with all Donor Human Milk Banking Guidelines (NICE,HMBANA,EMBA) for the establishment and operation of human milk banks. In particular the requirements for rapid cooling defined as the milk temperature drop from 62.5°C (°F144.5 to °F77) in less than 10 minutes, with a resultant temperature of <4°C (°F39.2) within the pasteurisation cycle and validated accordingly. This is achieved prior to refrigeration of the feeds for storage.

Pasteurisation is also recommended when preparing special diets for paediatric use. Pathogens could be introduced during the feed preparation. For this a special cycle of 67°C (°F152.6) for 4 minutes is used. (Current practice proven at Great Ormond Street Hospital and many Special Feeds Units). Pasteurisers are in use in Neonatal Intensive Care Units, Central Milk Banks and Paediatric Milk Kitchens and Special Feeds Units, world-wide.

The S90 ECO represents the latest generation of infant feed pasteurisers, co-invented by Professor JD Baum and developed by DJ Colgate with valuable input from Neonatologists, Microbiologists and Dieticians, having undergone continuous research and development from early 1980.

The new features include:

- Greater accuracy of pasteurisation times & temperatures
- System diagnostics
- Reduced cycle time

STERIFEED
.com

Medicare Colgate Ltd
Post Cross Business Park, Cullompton, Devon,
EX15 2BB, England
Tel: 00 44 1884 266 666 Fax: 01884 266 333
E-mail info@sterifeed.com
web www.sterifeed.com

CARING FOR YOUR BABY



S90 ECO

Pasteurisers for Donor Human Milk & Special Diets



Greater accuracy of pasteurisation times and temperatures

The control of the pasteurisation cycle was previously achieved by measuring the bath temperature and using this to discern the temperature of the feed in the bath. This can lead to longer cycle times to ensure the various quantities of milk have been treated.

The S90 Eco uses a microprocessor to control the pasteurisation cycle via the ACTUAL temperature of the milk assisted by the external probe in the control bottle. This results in very accurate cycles, both in terms of pasteurisation control and cooling set points. It also is extremely efficient in dealing with load variation.

Reduced cycle time

The cycle time is 30-40 minutes shorter on the ECO.

Process Verification: The Sterifeed Data Logger requires no direct connection to a PC. The reading is taken every minute, recording the exact temperature of the milk, time and date. This information is downloaded on to the software provided to give a permanent record of satisfactory treatment for every batch. Which can be printed in either graph or list format so that proof of treatment can be provided at any time.

Bottles: The Sterifeed, smooth necked range of clear storage bottles is recommended for use with this equipment. Either an integral seal or an induction safety seal is suitable. These bottles are sterile for single use but can be re-used using dishwashing equipment with a disinfectant cycle.


Baskets: Flexible Basket options available for all bottle sizes.

General Features:

- Fully automatic operation
- Programme selection to give specified temperature and times which are normally between 62.5°C – 63°C (145.4F) x 30 mins for mothers' milk, 67°C (152.6F) x 4 mins for special feeds
- Rapid, precise cooling of feeds to 4°C (39.2F) in approximately 20 minutes
- Cycle will depend on the temperature of the incoming hot water supply
- Programme Logic Control (PLC) to facilitate any future changes to time and temperature.
- Visual fault finder

Safety Features:

- Audible and visual alarm for any variations.
- Feeding bottles are submerged during the heating cycle to ensure milk droplets in the neck and cap area receive the same precise treatment as the bulk of the feed (**recommended by the Health Protection Agency & The Human Milk Banking Association of North America Guidelines for the Establishment & Operation of a Donor Human Milk Bank**)
- Bottles are not submerged during cooling process when a vacuum occurs (unless safety seals are in use)
- No residue water traps eliminating equipment sterilisation cycle.

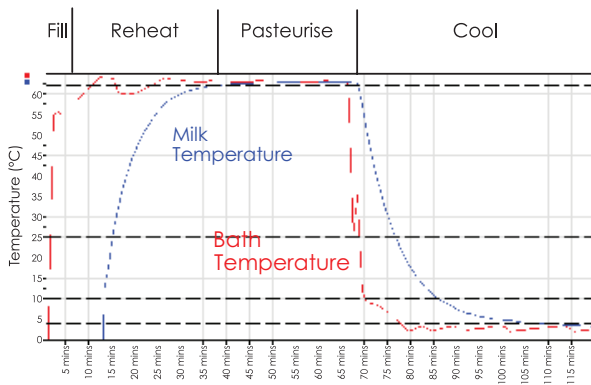

Time and temperature graph at 62.5°C for 30 minutes

Specifications

Dimensions/mm	600W x 700D x 920H
Chamber/mm	400L x 400W x 250H – 40 litres
Electrical	230v/1Ph/50Hz - 2800 watts
Full Load Current	12.5A
Electrical Consumption	1.83 kWh
Internal Control Voltage	230v/24v
Capacity	9.36 litres (36x130ml, 36x250ml, 96x50ml, 72x130ml with foil seals)
Water Consumption	85 litres
Noise level	45 dBA@1m
Heat output during cooling	1.7 kWh

All models are available in 50 Hz & 60 Hz

Harmonized Standards	BS EN 60204-1:2006 & A1:2009, BS EN 12100-1:2003, BS EN 61000-2-2, BS EN 61000-2-4
CE Directives	2006/95/EC
CSA	approved
Construction	Stainless steel

Guarantee: The pasteurisers are guaranteed against faulty materials and workmanship for a period of one year.



Distributed by:

CARING FOR YOUR BABY

